



CERTIFICATE OF ACCREDITATION

The ANSI National Accreditation Board

Hereby attests that

Athamas Sale & Service Co., Ltd
254/152 Ramkhamhaeng 112 Rd.
Sapansoong, Bangkok, 10240, Thailand

Fulfills the requirements of

ISO/IEC 17025:2017

In the field of

CALIBRATION

This certificate is valid only when accompanied by a current scope of accreditation document.
The current scope of accreditation can be verified at www.anab.org.

Jason Stine, Vice President

Expiry Date: 11 July 2027

Certificate Number: AC-3401



This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017.
This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory
quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).

SCOPE OF ACCREDITATION TO ISO/IEC 17025:2017

Athamas Sale & Service Co., Ltd

254/152 Ramkhamhaeng 112 Rd.
Sapansoong, Bangkok, 10240, Thailand

Mr. Nontiwat Phuwaratphanuphat
nontiwat@athamas-tha.com
+66988945465

CALIBRATION

ISO/IEC 17025 Accreditation Granted: 11 July 2025

Certificate Number: **AC-3401** Certificate Expiry Date: **11 July 2027**

Chemical Quantities

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
pH Meter ¹	pH 4 pH 7 pH 10	0.021 pH 0.021 pH 0.021 pH	Comparison to pH Buffer Solutions
Conductivity Meter ¹	84 µS/cm 1 413 µS/cm 12 880 µS/cm	0.84 µS/cm 7.1 µS/cm 0.07 mS/cm	Comparison to Conductivity Buffer Solutions

Electrical – DC/Low Frequency

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Voltage - Source ¹	(-10 to 100) mV (> 0.1 to 1) V (> 1 to 10) V	0.08 mV 0.013 V 0.009 V	Comparison to Multifunction Process Calibrator Fluke 701
DC Current - Source ¹	(2 to 22) mA	0.015 mA	Comparison to Multifunction Process Calibrator Fluke 701

Electrical – DC/Low Frequency

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Resistance - Source ¹	Up to 10 Ω (> 10 to 100) Ω (> 0.1 to 1) k Ω (> 1 to 5) k Ω (> 5 to 10) k Ω	0.064 Ω 0.12 Ω 0.008 k Ω 0.017 k Ω 0.024 k Ω	Comparison to Multifunction Process Calibrator Fluke 701
DC Voltage - Measure ¹	Up to 10 mV (> 10 to 50) mV (> 50 to 100) mV (> -1 to 1) V (> 1 to 10) V (> 10 to 30) V	0.028 mV 0.05 mV 0.078 mV 0.012 V 0.017 V 0.038 V	Comparison to Multifunction Process Calibrator Fluke 701
DC Current – Measure ¹	(-30 to 0) mA (> 0 to 4) mA (> 4 to 20) mA (> 20 to 30) mA	0.019 mA 0.012 mA 0.017 mA 0.019 mA	Comparison to Multifunction Process Calibrator Fluke 701
Resistance – Measure ¹	Up to 10 Ω (> 10 to 50) Ω (> 50 to 100) Ω (> 100 to 500) Ω (> 500 to 1 000) Ω (> 1 to 4) k Ω	0.07 Ω 0.12 Ω 0.17 Ω 1.2 Ω 1.7 Ω 0.6 k Ω	Comparison to Multifunction Process Calibrator Fluke 701
Electrical Simulation of RTD Indicating Devices – Source/Measure PT385 (100 Ω) ¹	PT385 (100 Ω) (-200 to 0) $^{\circ}\text{C}$ (> 0 to 300) $^{\circ}\text{C}$ (> 300 to 800) $^{\circ}\text{C}$	0.8 $^{\circ}\text{C}$ 1 $^{\circ}\text{C}$ 1.4 $^{\circ}\text{C}$	Comparison to Multifunction Process Calibrator Fluke 701

Electrical – DC/Low Frequency

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Electrical Simulation of Thermocouple Indicating Devices – Source/Measure ¹	Type K		Comparison to Multifunction Process Calibrator Fluke 701
	(-200 to 0) °C	1.1 °C	
	(> 0 to 300) °C	0.6 °C	
	(> 300 to 500) °C	0.8 °C	
	(> 500 to 1 300) °C	1.1 °C	
	Type T		
	(-200 to 0) °C	1.0 °C	
	(> 0 to 200) °C	0.9 °C	
	(> 200 to 400) °C	0.6 °C	
	Type J		
	(-200 to 0) °C	0.9 °C	
	(> 0 to 300) °C	0.6 °C	
	(> 300 to 1 200) °C	0.8 °C	
	Type E		
	(-200 to 0) °C	1.7 °C	
	(> 0 to 500) °C	0.6 °C	
	(> 500 to 1 000) °C	0.7 °C	
	Type R		
	(0 to 300) °C	2.9 °C	
	(> 300 to 1 700) °C	1.5 °C	
	Type S		
	(0 to 300) °C	2.9 °C	
	(> 300 to 800) °C	1.3 °C	
	(> 800 to 1 700) °C	1.5 °C	

Mass and Mass Related

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Mass Determination	1 kg 2 kg 5 kg 10 kg 20 kg	8.2 mg 16 mg 36 mg 0.3 g 0.32 g	Comparison to Weights Set / Electronic Balance
Scales and Balances ¹			
Resolution 0.0001 g	50 mg to 50 g (50 to 100) g (100 to 200) g (200 to 300) g	0.4 mg 0.7 mg 1.4 mg 2.1 mg	Comparison to Weights Set
Resolution 0.001 g	(> 300 to 500) g (> 500 to 1 000) g (> 1 to 1.5) kg (> 1.5 to 2) kg (> 2 to 3) kg (> 3 to 5) kg (> 5 to 10) kg (> 10 to 15) kg (> 15 to 20) kg	4 mg 7 mg 10 mg 14 mg 21 mg 34 mg 69 mg 0.1 g 0.14 g	
Scales and Balances ¹			
Resolution 0.01 kg	(> 20 to 30) kg (> 30 to 100) kg (>100 to 150) kg (> 100 to 200) kg (> 200 to 300) kg (> 300 to 500) kg (> 500 to 750) kg (> 750 to 1 000) kg	10 g 12 g 13 g 15 g 20 g 30 g 45 g 59 g	Comparison to Weights Set

Mass and Mass Related

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Gauge Pressure – Analog and Digital Pressure Gauges, Pressure Transducers, Pressure Transmitters, Differential Pressure Gauges, Manometers, Pressure Switches (Pneumatic & Hydraulic) ¹	(0 to 2 000) kPa (0 to 140) bar (> 140 to 700) bar	0.75 kPa 0.17 bar 0.81 bar	Comparison to Digital Pressure Indicator PC6-PRO-0020 and Digital Test Gauge XP2i
Vacuum Gauge ¹	(-0.90 to 0) kPa	0.04 kPa	Comparison to Digital Pressure Indicator PC6-PRO-0020

Thermodynamic

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Air Temperature Controlled, Chamber, Hot Air Oven ¹	(25 to 250) °C	0.2 °C	Comparison to Data Acquisition/Switch Unit w/Sensor
Incubator ¹	(10 to 150) °C	0.2 °C	Comparison to Data Acquisition/Switch Unit w/Sensor
Refrigerator & Freezer ¹	(-40 to 10) °C	0.2 °C	Comparison to Data Acquisition/Switch Unit w/Sensor
Autoclave ¹	100 °C (110 to 135) °C	0.54 °C 0.63 °C	Comparison to Data Acquisition/Switch Unit w/Sensor
Liquid Bath, Water Bath ¹	(-40 to 150) °C	0.23 °C	Comparison to Data Acquisition/Switch Unit w/ RTD Sensor


Thermodynamic

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Dial Thermometer ¹	(-40 to 200) °C (> 200 to 400) °C (> 400 to 450) °C (> 450 to 650) °C	0.046 °C 0.053 °C 2 °C 2.5 °C	Comparison to Temperature Indicator with PRT Standard DT I1000, Fluke 741 with thermocouple Type S
Thermocouple Probe Types K, J, E, T, N, R, S ¹	(-40 to 200) °C (> 200 to 400) °C (> 400 to 450) °C (> 450 to 1 100) °C	0.089 °C 0.093 °C 2 °C 2.5 °C	Comparison to Temperature Indicator with PRT Standard DTI1000, Fluke 741 with thermocouple Type S
Thermocouple Probe Types RTD ¹	(-40 to 200) °C (> 200 to 400) °C	0.089 °C 0.093 °C	Comparison to Temperature Indicator with PRT Standard DTI1000
Digital Thermometer With Sensor Types K, J, E, T, N, R, S ¹	(-40 to 200) °C (> 200 to 400) °C (> 400 to 450) °C (> 450 to 1 100) °C	0.046 °C 0.053 °C 2 °C 2.5 °C	Comparison to Temperature Indicator with PRT Standard DTI1000, Fluke 741 with Thermocouple Type S
Digital Thermometer With Probe Type RTD ¹	(-40 to 200) °C (> 200 to 400) °C	0.046 °C 0.053 °C	Comparison to Temperature Indicator with PRT Standard DTI1000
Liquid-in-Glass Thermometers ¹	(-20 to 150) °C	0.07 °C	Comparison to Temperature Indicator with PRT Standard DTI1000

Calibration and Measurement Capability (CMC) is expressed in terms of the measurement parameter, measurement range, expanded uncertainty of measurement and reference standard, method, and/or equipment. The expanded uncertainty of measurement is expressed as the standard uncertainty of the measurement multiplied by a coverage factor of 2 ($k=2$), corresponding to a confidence level of approximately 95%.

Notes:

- On-site calibration service is available for this parameter, since on-site conditions are typically more variable than those in the laboratory, larger measurement uncertainties are expected on-site than what is reported on the accredited scope.

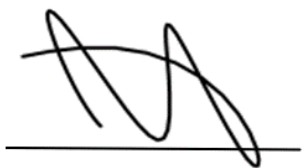

Jason Stine, Vice President